RETURN TO PRODUCT BULLETIN TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

PRODUCT BULLETIN

Product(s):	Narkomed® 6000 Series
Bulletin Number:	134
Release Date:	6/11/02
Pages:	3

Subject: Auxiliary Video Output - Narkomed 6000 Series

The auxiliary video output feature is now released and available for purchase on the Narkomed 6000 series system. This feature provides the ability to connect an additional display to the NM6000, offering easy viewing of monitoring information for surgeons and other OR personnel. The remote display monitor can be mounted on top of the Narkomed 6000 or in other remote locations. The basic features of the auxiliary output include:

- Information presented on the remote display is an exact duplicate of the NM6000 main display (the remote display is non-configurable)
- Up to three displays can be connected to each NM6000
- The machine and wall mounting options provide display movement of 180° side to side rotation and +/- 45° up/down tilt
- The auxiliary output feature can be added to any NM6000 series flat panel system

Due to varying needs, the auxiliary video option can be configured to meet the specific requirements of each customer. The basic components of this feature are as follows:

Name	Part Number	Description	List Price
Common Parts Kit **(Required)**	#4117799	Internal hardware, making the NM6000 remote display "ready". This includes three video output connectors on the back panel of the NM6000.	$1,000
Machine Mount Kit (Optional)	#4117801	GCX rail and mounting kit to attach the auxiliary display to the top of the NM6000. Isolation transformer is included in this kit.	$1,125
Wall Mount Kit (Optional)	#4117800	GCX rail and mounting kit to attach the auxiliary display to any wall. Isolation transformer is included in this kit.	$1,125

Customers are not required to purchase a mounting kit from Dräger. They are free to purchase and configure any mounting system they prefer. Additionally, the Wall Mount kit purchased from Dräger will need to be installed by the customer. Dräger Service cannot be responsible for mounting any display off the machine.

For any remote mounting, cabling may be necessary to connect the auxiliary display to the NM6000. The cabling may be purchased from Dräger. The part numbers are as follows:

Name	Part Number	List Price
50 ft. Video Cable	#4117781-050	$100
100 ft. Video Cable	#4117781-100	$135

For the customer who requires the complete solution, we are also offering a 20 inch, NEC model #LCD2010x
full-color flat panel display as an option.

Name	Part Number	List Price
NEC 20" Flat Panel Display (non-medical grade)	#4117789	$5,250
Isolation Transformer	#4114985	$765

Note: To prevent excess leakage current, any non-medical grade display requires the use of an isolation transformer. Up to three displays can be connected to each NM6000. In the event that more than one display is configured, an isolation transformer is required for each display.

Please refer to the flow diagram on the following page to help you determine which options are needed to meet the needs of your customer.

Installation
The Auxiliary Video Output will be a field installation only. Standard Service Labor & Travel charges apply. New NM6000's ordered with this feature will be configured at the customer site.

Additional Information
For customers who wish to purchase a remote display monitor on their own, please refer to the *Specifications for Flat Panel Display for Auxiliary Video Output* posted on the Marketing Library. This document lists the specific requirements that a display must meet to ensure compatibility with the NM6000's auxiliary video option.

Please contact Mary Kyryk at ext. 2619 or kyrykm@draegermed.com if you have any additional questions.

Auxiliary Video Output Option Ordering Decision Tree

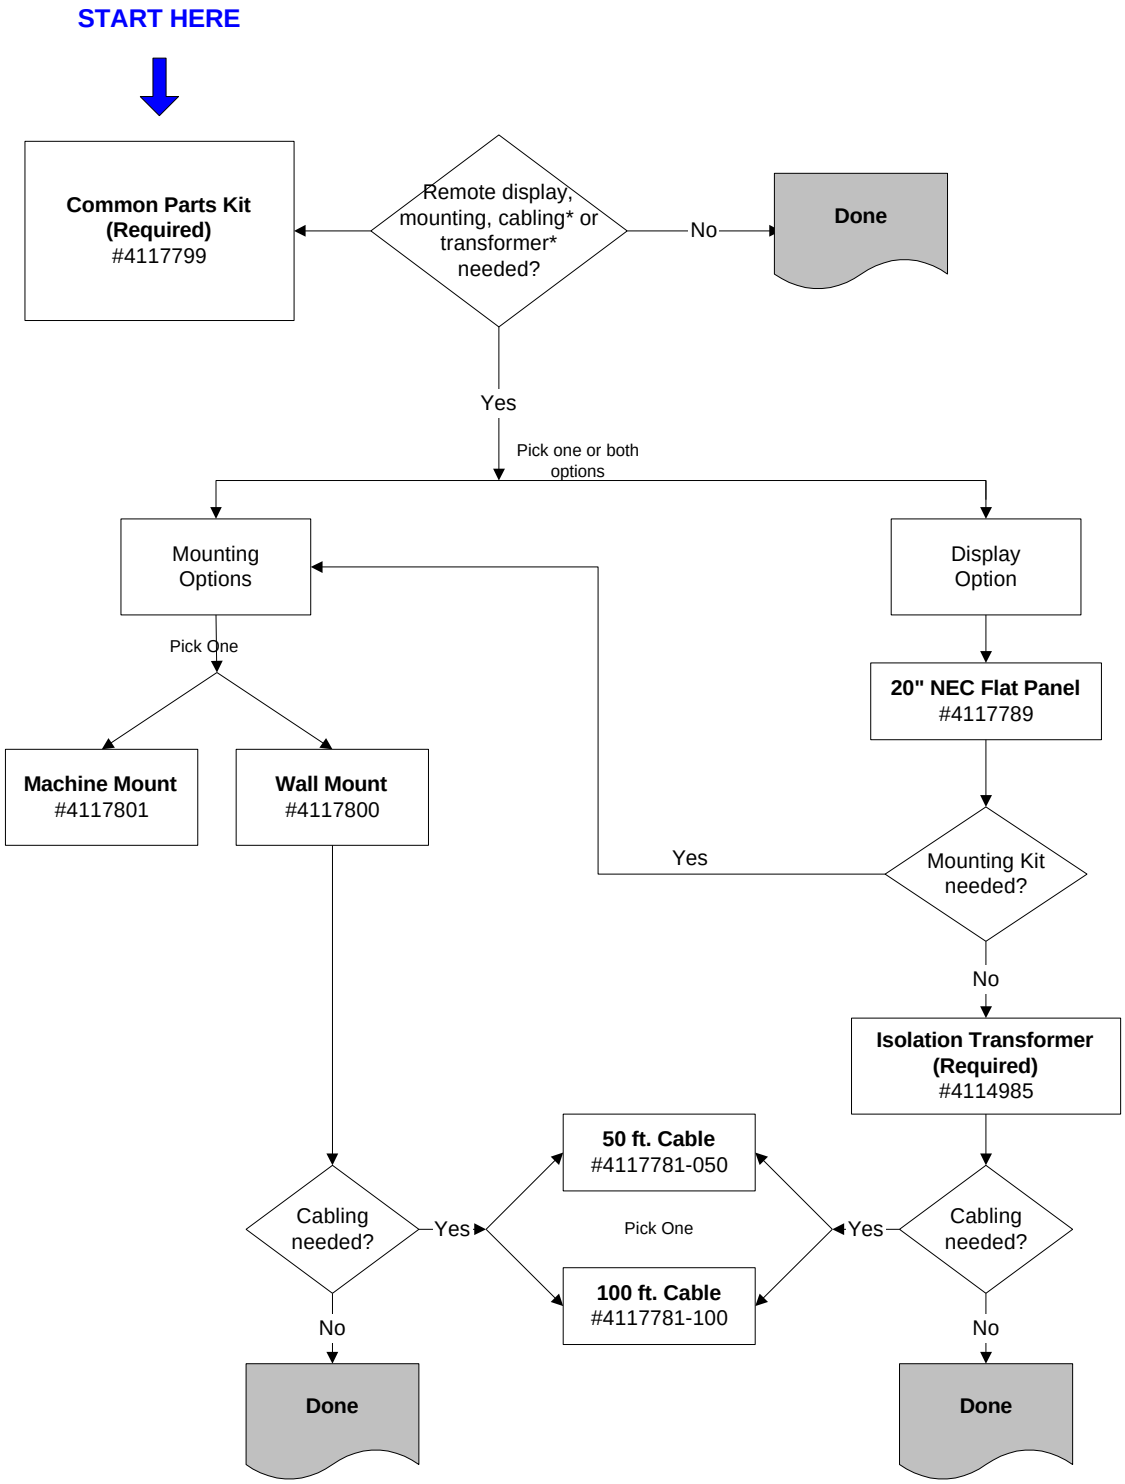

*__Note:__ The Cables and Isolation Transformer can be ordered separately for those customers who need only these components.